

A QbD with Design-of-Experiments Approach to the Development of a Chromatographic Method for the Separation of Impurities in Vancomycin

Peter G. Alden, Warren Potts, and Dana Yurach
Waters Corporation, Milford, MA, U.S.

APPLICATION BENEFITS

Using specialized software in conjunction with UPLC® Technology, an optimized QbD method for the impurities in vancomycin can be developed that will be robust for method validation and transfer.

WATERS SOLUTIONS

ACQUITY UPLC®

Fusion Method Development

Empower™ 2 CDS

KEY WORDS

Quality by design (QbD),
method development,
design of experiment (DOE)

INTRODUCTION

Analytical methods are developed at various stages of the drug development process for samples of varying complexity. Due to the inherent nature of the method development process, redundant efforts take place across an organization, resulting in a very costly and time-consuming activities. If we can streamline the process by which we develop methods, products can be brought to market faster and in a more cost effective manner.

Many different approaches are typically used to develop chromatographic methods today including trial and error, method/column scouting, and software approaches such as first principles approaches and simplex optimization procedures. All these approaches suffer from the inability to determine complex interactions effects between method variables or measurably consider method robustness during the method development process.

Vancomycin is a tricyclic glycopeptide antibiotic derived from *Amycolatopsis orientalis* (formerly *Nocardia orientalis*) and is indicated for the treatment of serious or severe infections caused by susceptible strains of methicillin-resistant (beta-lactam-resistant) staphylococci. Vancomycin is a large molecule (MW 1485.71 daltons) and contains many impurities that are difficult if not impossible to separate. Traditional HPLC gradient methods have shown the ability to separate out as many as 13 of these impurities, while the use of sub-2- μm ACQUITY UPLC Column chromatography has demonstrated the separation of as many as 26 impurities.

This paper describes a novel method development approach using Quality by Design (QbD) with Design of Experiments to develop a UPLC method for separating 39 impurities in vancomycin resulting in an optimally performing analytical method while simultaneously applying robustness limits to ensure success in final method validation and ultimately in method transfer.

EXPERIMENTAL

Analytical instrumentation

The vancomycin studies described here were carried out using an automated integrated system consisting of Fusion Method Development Software, Empower 2 Chromatography Data Software (CDS), and an ACQUITY UPLC System with PDA, Column Manager, and Solvent Select Valve allowing for the screening of up to four different column chemistries, six different aqueous buffers/pHs, and two different organic mobile phases in one run.

Data management

Fusion Method Development Software (S-Matrix Corporation, Eureka, CA) is a Quality by Design based LC Method Development software package with built-in robustness metrics. Fusion includes a built-in interface with the Empower 2 CDS Software that controls the ACQUITY UPLC System. Using the chromatographic results collected from Empower 2 CDS, Fusion manages complex statistics and models for method optimization. Fusion builds experiments, analyzes data, and presents results as visual and numerical method predictions.

RESULTS AND DISCUSSION

Phase 1: Rapid screening

Experiment design

The first phase of the method development involves the screening of the major effectors of selectivity, primarily the column chemistry, buffer pH, and organic mobile phase. The variables and ranges screened along with the constant conditions are listed in Figure 1's tables.

Column Assignments		Reservoir Assignments		Experiment Constants	
Column Valve Position	Column Level	Reservoir A1-1	Level	Constant Name	Constant Value
ValvePosition_1	BEH C18, 2.1x100mm, 1.7um	pH	3.0	Sample Concentration	0.25
ValvePosition_2	BEH RP18, 2.1x100mm, 1.7um	Reservoir A1-2	Level	Pump Flow Rate	0.450
ValvePosition_3	BEH RPwyl, 2.1x100mm, 1.7um	pH	5.0	Injection Volume	2.5
ValvePosition_4	BEH C8, 2.1x100mm, 1.7um	Reservoir A1-3	Level	Oven Temperature	45.0
		pH	6.5	Wavelength	254
		Reservoir A2	Level	Equilibration Time	10.0
		Aqueous Solution	---	Equilibration % Organic	2.0
		Reservoir B1	Level	Initial Hold Time	1.0
		Acetonitrile	---	Initial Hold % Organic	2.0
		Reservoir B2	Level	Final Hold Time	2.0
		Methanol	---	Final Hold % Organic	40.0
				Ramp Up to Wash Time	0.1
				Column Wash Time	2.0
				Column Wash % Organic	95.0
				Ramp Down from Wash Time	0.1
				Re-equilibration Time	1.0
				Re-equilibration % Organic	95.0

Figure 1. Screened variables and ranges.

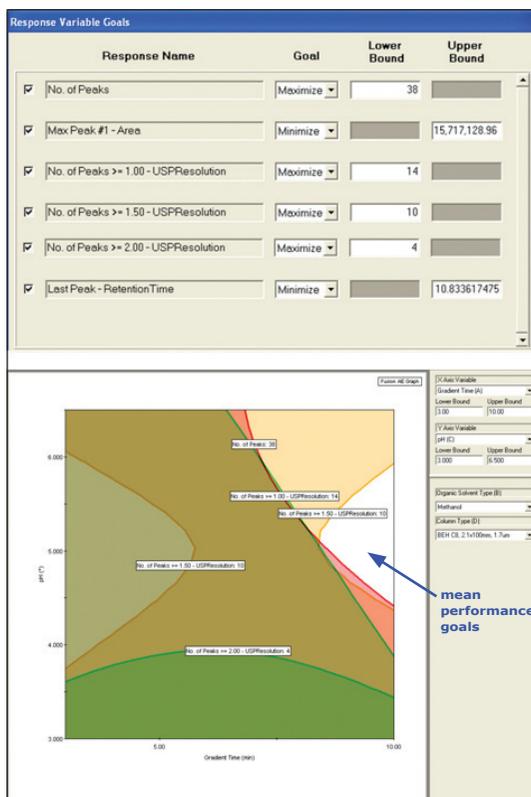


Figure 2. Processed data are imported to Fusion, where an overlay graph illustrates in white the region where the mean performance goals are achieved.

Overlay graphics

The experimental design is run and data processed on the chromatographic system and the results are imported back into Fusion. The software predicts the optimum LC method after modeling all significant effects – linear, interaction, and complex – on each critical method performance characteristic. The unshaded (white) area of the overlay graph shown for the BEH C₈ column with methanol as the organic mobile phase (Figure 2) highlights the experimental region where the mean performance goals are obtained.

Optimization

The Automated Optimizer wizard defines the LC method performance goals and ranks them in order of importance. The software searches for the LC method that meets all the performance goals simultaneously. The best result(s) are reported along with predicted results for an experimental run (Figure 3). These conditions are used for the next stage, Method Optimization.

Optimize Responses - Response Variable Goals

Response Name	Goal	Lower Bound	Upper Bound	Relative Rank
<input checked="" type="checkbox"/> No. of Peaks	Maximize	35	45	1
<input checked="" type="checkbox"/> Max Peak #1 - Area	Minimize	5,455,220.57137	15,717,128.9631	0.5
<input checked="" type="checkbox"/> No. of Peaks >= 1.00 - USPRResolution	Maximize	12	17	0.5
<input checked="" type="checkbox"/> No. of Peaks >= 1.50 - USPRResolution	Maximize	8	12	0.4
<input checked="" type="checkbox"/> No. of Peaks >= 2.00 - USPRResolution	Maximize	4	8	0.2
<input checked="" type="checkbox"/> Last Peak - RetentionTime	Minimize	3.244845902	10.833617475	0.4

Confidence Limits for the Predicted Response(s) ± 2 Sigma

Optimizer Answer #1: 34 of 34

Study Variable Data

Study Variable Name	Optimizer Answer Level Setting
Gradient Time	10.00
Organic Solvent Type	Methanol
pH	5.543
Column Type	BEH C8, 2.1x100mm, 1.7um

Best conditions from rapid screen runs

Predicted Response Data

Response Variable Name	Target	Optimizer Answer Predicted Response	-2 Sigma Confidence Limit	+2 Sigma Confidence Limit	Relative Rank
No. of Peaks	Maximize	42.21	36.54	47.87	1.0
Max Peak #1 - Area	Minimize	10,802,293.47829680000	7,112,353.74702277000	14,492,233.20957080000	0.5
No. of Peaks >= 1.00 - USPRResolution	Maximize	16.36	11.55	21.17	0.5
No. of Peaks >= 1.50 - USPRResolution	Maximize	10.95	8.65	13.26	0.4
No. of Peaks >= 2.00 - USPRResolution	Maximize	8.78	5.57	12.70	0.2
Last Peak - RetentionTime	Minimize	9.11778162928	8.39564415224	9.90124127730	0.4

Figure 3. Fusion's Automated Optimizer facilitates determination of the LC method that meets all performance goals.

Design Variables

Variable	Range
Pump Flow Rate	0.25 - 0.45 mL/min
Gradient Time	6.0 - 10.0 min
Final % Organic	25% - 40% B
Column Temperature	35 - 60 °C

Reservoir Assignments

Reservoir A1-1	Level
pH	5
Reservoir A2	Level
Aqueous Solution	---
Reservoir B2	Level
Methanol	---

Experiment Constants

Constant Name	Constant Value
Column Type	BEH C8 100mm
Injection Volume	2.5
Wavelength	254
pH	5.0
Initial % Aqueous	95
Initial % Organic	5
Equilibration Time	10.0
Equilibration % Organic	5.0
Initial Hold Time	1.0
Final Hold Time	2.0
Ramp Up to Wash Time	0.1
Column Wash Time	2.0
Column Wash % Organic	95.0
Ramp Down from Wash Time	0.1
Re-equilibration Time	1.0
Re-equilibration % Organic	5.0

Figure 4. Fusion determines optimal method conditions and exports this information back to Empower 2 to be run and processed.

Phase 2: Method optimization

Experiment design

Phase 2 experiments use the column (ACQUITY UPLC BEH C8, 2.1 x 100 mm, 1.7 μ m) and mobile phase (pH 5.0 buffer, methanol B solvent) results from Phase 1 plus additional variables with tighter ranges to determine the optimum LC method. The experimental design is created using pump flow rate, gradient time, final percent organic, and column temperature as final optimization variables in the ranges shown (Figure 4).

Fusion Software creates the experimental design and exports it to Empower 2, automatically creating all the necessary instrument methods, method sets, and sample sets. The experimental design is run and data processed on the chromatographic system and the results are imported back into Fusion.

In addition to the data analysis for method optimization, Fusion applies a combination of Monte Carlo Simulation and Process Capability statistics to evaluate method flow robustness without running additional experiments.

Multiple response surface plots

Visualizing the results with Fusion's 3D Response Surface Plots demonstrates the combined effects of variables on key chromatographic responses such as resolution, peak tailing, and retention time. Colors represent the magnitude of interaction and the curvature indicates the type of interaction (Figure 5).

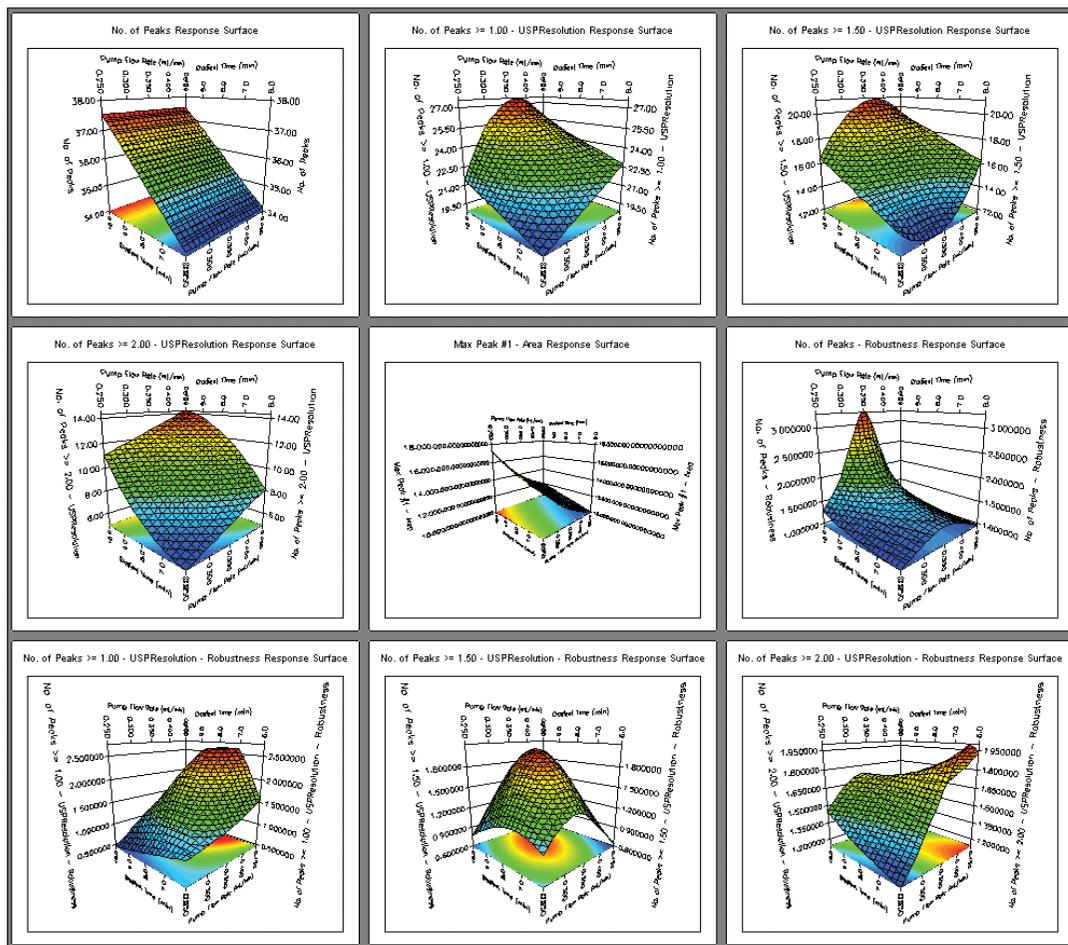


Figure 5. Surface plot responses.

Multiple response effects plots

Another option for visualizing the interactions between variables is through Multiple Response Effects Plots. These plots clearly identify simple linear additive effects (1), complex interactions of variables (2), and other types of response effects (Figure 6).

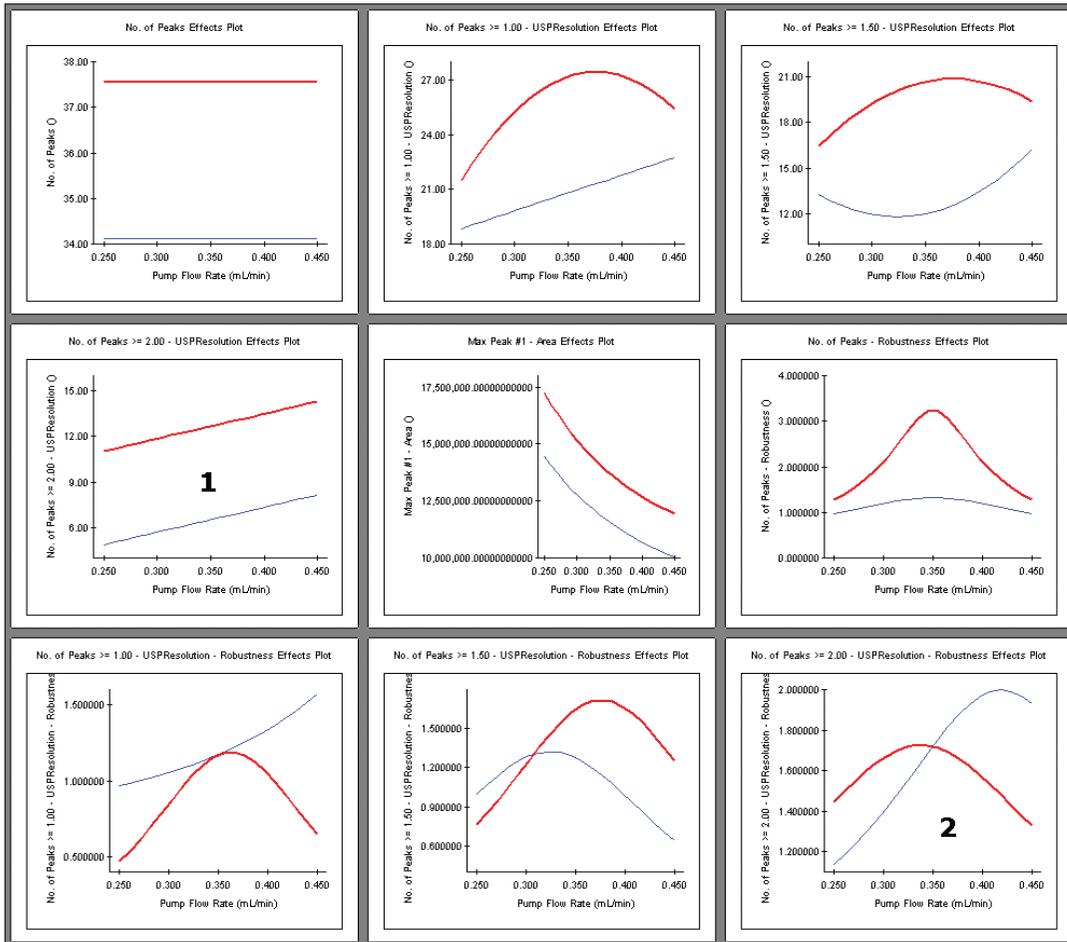


Figure 6. Effects plot responses.

Final results of method optimization

Next, an overlay graph is created using a number of critical chromatographic responses. Of primary importance for the vancomycin separation is maximizing the number of peaks observed and the number of peaks exceeding different levels of resolution while minimizing the area of the vancomycin peak, which equates to separating out the most impurities. The overlay graph shows the QbD Design Space (unshaded region) where the method meets the mean performance goals and robustness criteria (Figure 7).

Using ranked response variables, the Method Optimizer determines the optimum method to best meet the performance and robustness goals specified. The final method conditions are listed along with predicted response results with confidence limits for this method (Figure 8).

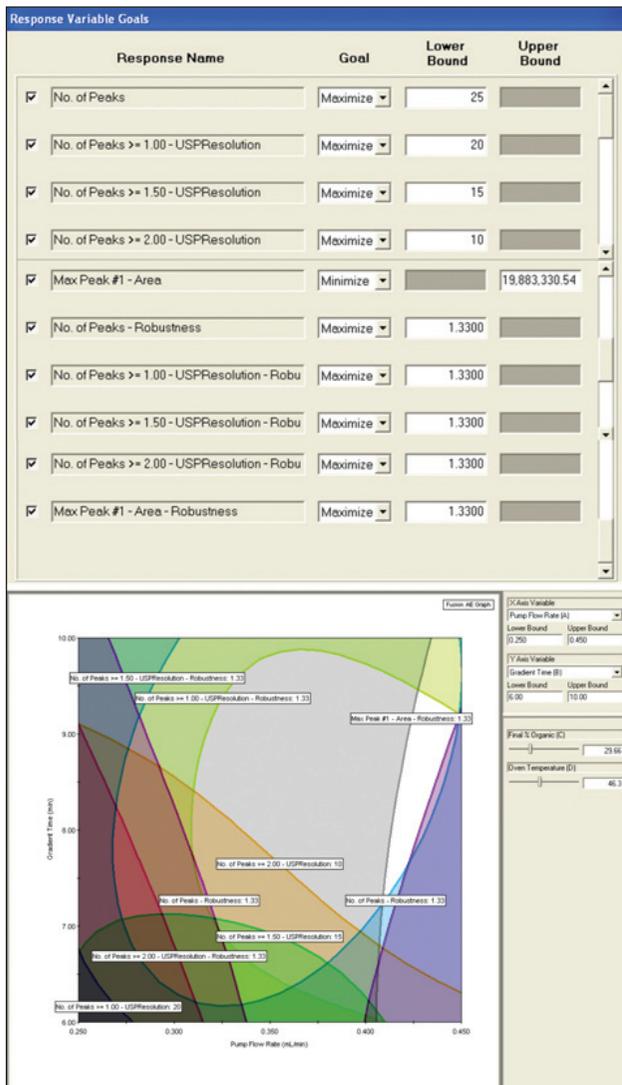


Figure 7. In the final overlay graph, the optimal QbD Design Space is the white or unshaded area.

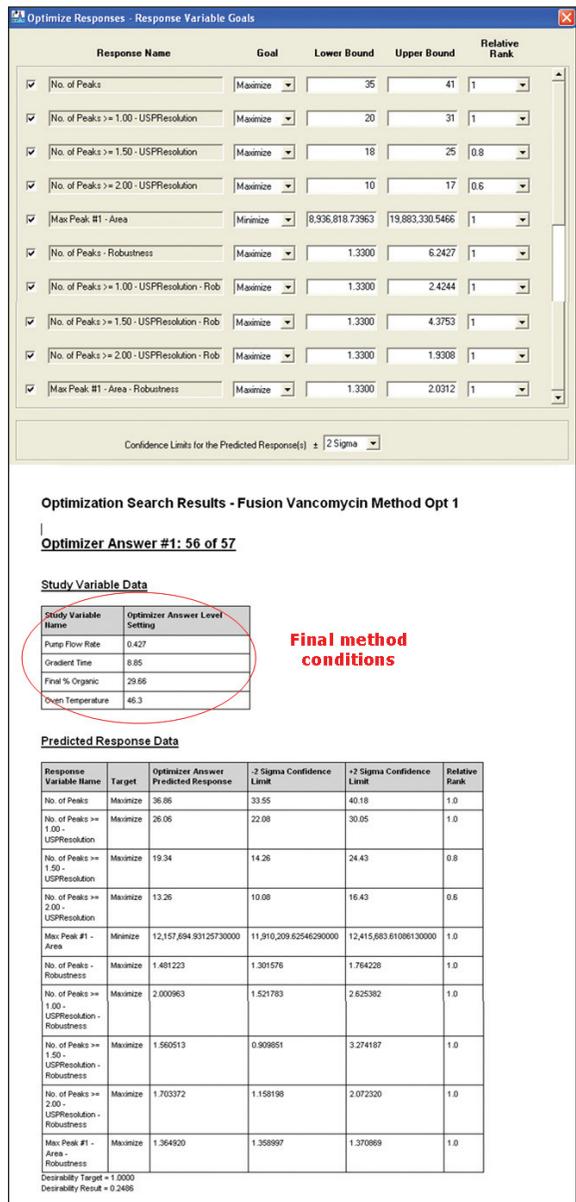


Figure 8. The Method Optimizer determines the optimum method to meet performance and robustness goals, and lists the final method and predicted responses.

Phase 3: Confirmation

Optimization results

The optimum method determined by the Fusion Method Optimizer was:

Column: ACQUITY UPLC BEH C₈ Column, 2.1 x 100 mm, 1.7 μm
Mobile phase A: 10 mM Ammonium Acetate, pH 5.0
Mobile phase B: Methanol
Flow rate: 0.427 mL/min
Gradient: 5% to 29.66% Methanol in 8.85 min
Column temp.: 46.3 °C

This method was exported to Empower 2 and the vancomycin sample was run to evaluate the prediction accuracy. The chromatogram in Figure 9 shows the separation of vancomycin impurities obtained with the optimized method.

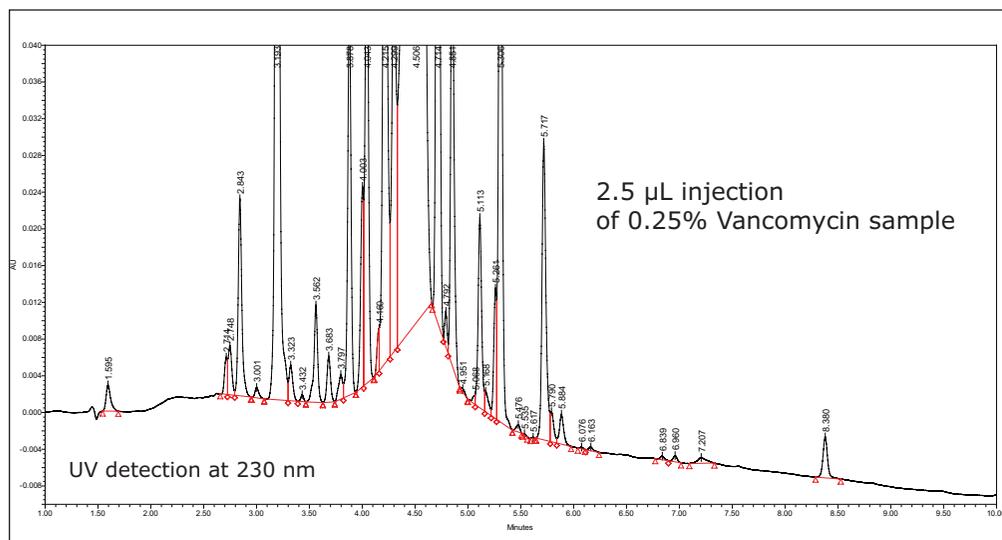


Figure 9. Confirmation run of the final UPLC method recommended by Fusion Software, where the number of impurities observed increased from 26 to 39.

The experimental results compare favorably with Fusion Software's predictions.

Response variable	Predicted response	Experimental response
# of Peaks	36.9 Peaks	39 Peaks
# of Peaks ≥ 1.0 Rs	26.1 Peaks	27 Peaks
# of Peaks ≥ 1.5 Rs	19.3 Peaks	18 Peaks
# of Peaks ≥ 2.0 Rs	13.3 Peaks	12 Peaks

The QbD-based Fusion Software method improved the separation of impurities in vancomycin from 26, obtained previously with UPLC methods developed manually, to 39 impurities observed with the method shown.

CONCLUSIONS

- Fusion Method Development Software, used with the ACQUITY UPLC System, generated an optimized method for the analysis of vancomycin and its impurities in two business days.
- The use of UPLC data managed and processed by Fusion and Empower 2 software established a valid design space with both mean performance (set point optimization) and robustness (operating space).
- The QbD method's resolution improved from 26 peaks in previous method to 39 peaks.
- Integrated robustness calculations ensure a reproducible method, which increases confidence in the ability to validate and transfer that method.

Waters

THE SCIENCE OF WHAT'S POSSIBLE.™

Waters, UltraPerformance LC, UPLC, and ACQUITY UPLC are registered trademarks of Waters Corporation. Empower and The Science of What's Possible are trademarks of Waters Corporation.

S-Matrix is a registered trademark of S-Matrix Corporation. Fusion Method Development is a trademark of S-Matrix Corporation. All other trademarks are the property of their respective owners.

©2010 Waters Corporation. Printed in the U.S.A.
September 2010 720003719EN LL-LCGC

Waters Corporation
34 Maple Street
Milford, MA 01757 U.S.A.
T: 1 508 478 2000
F: 1 508 872 1990
www.waters.com



S-Matrix Corporation
1594 Myrtle Avenue
Eureka, CA 95501 U.S.A.
www.smatrix.com

